

1/7

FIG.1

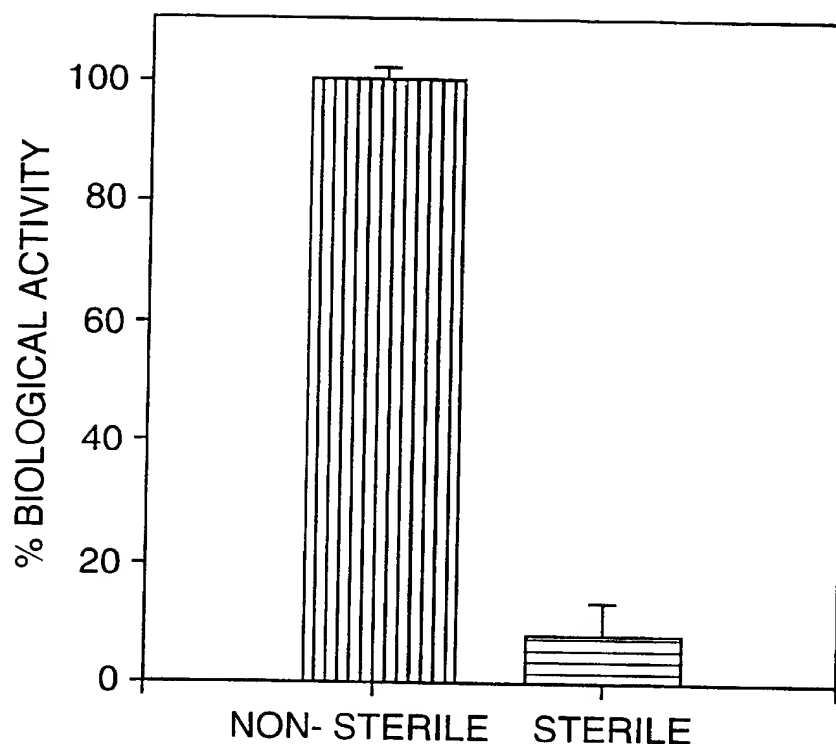


FIG.2

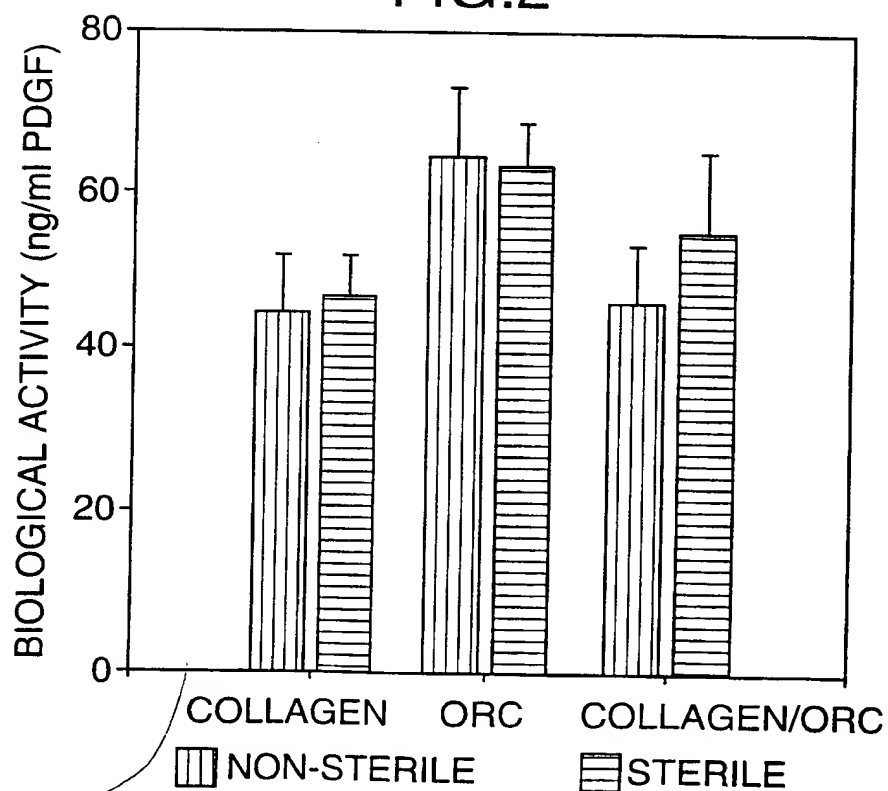


FIG. 3

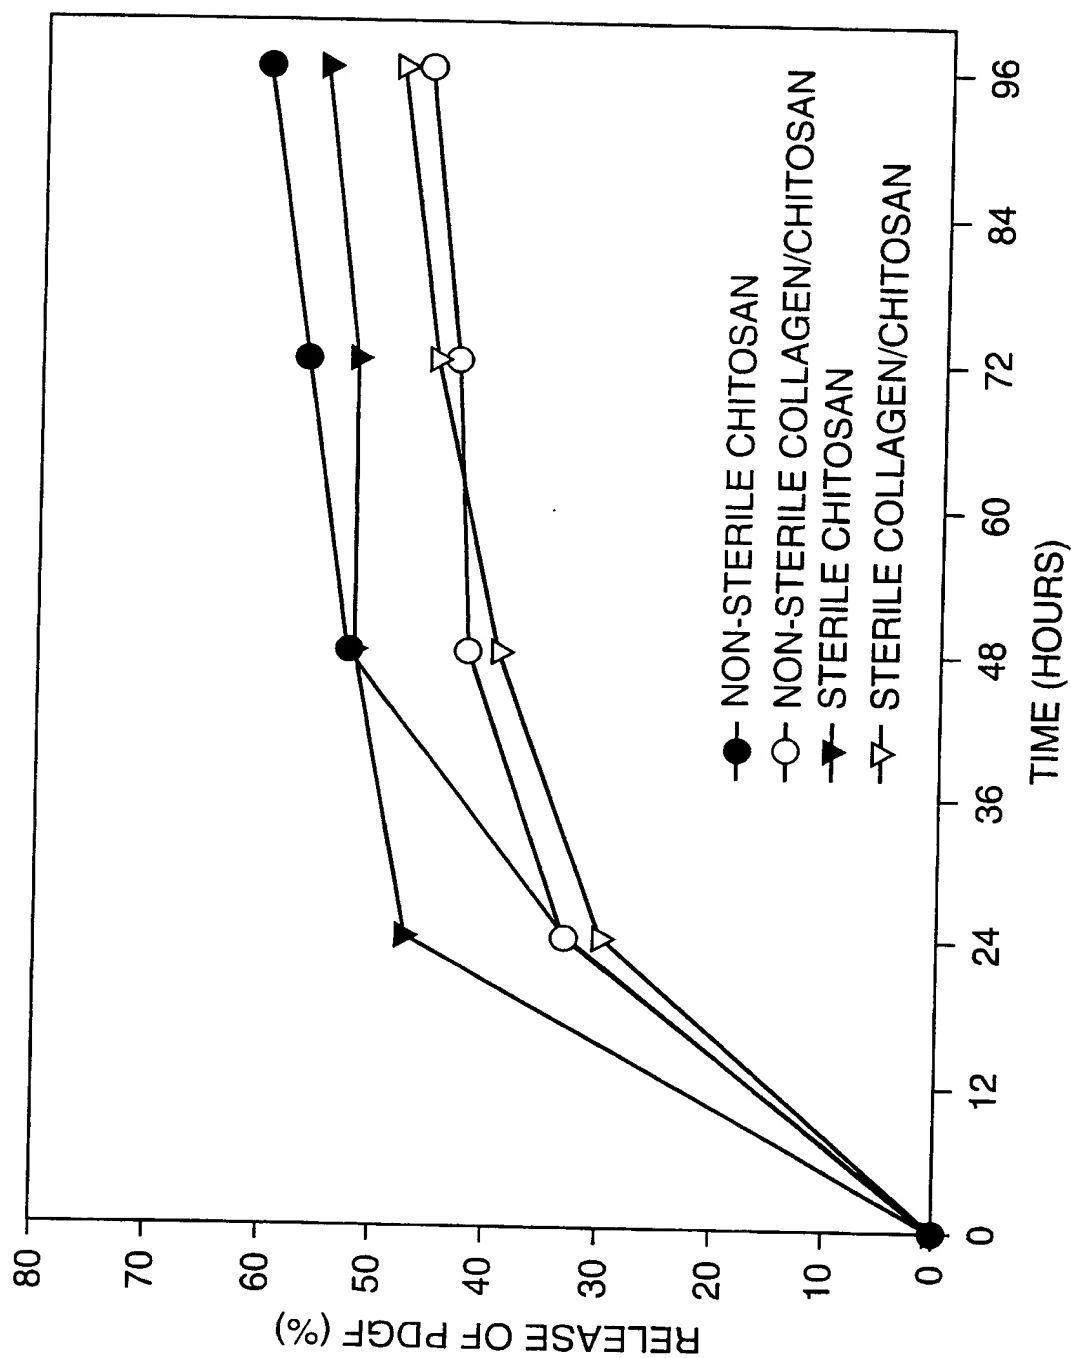


FIG. 4


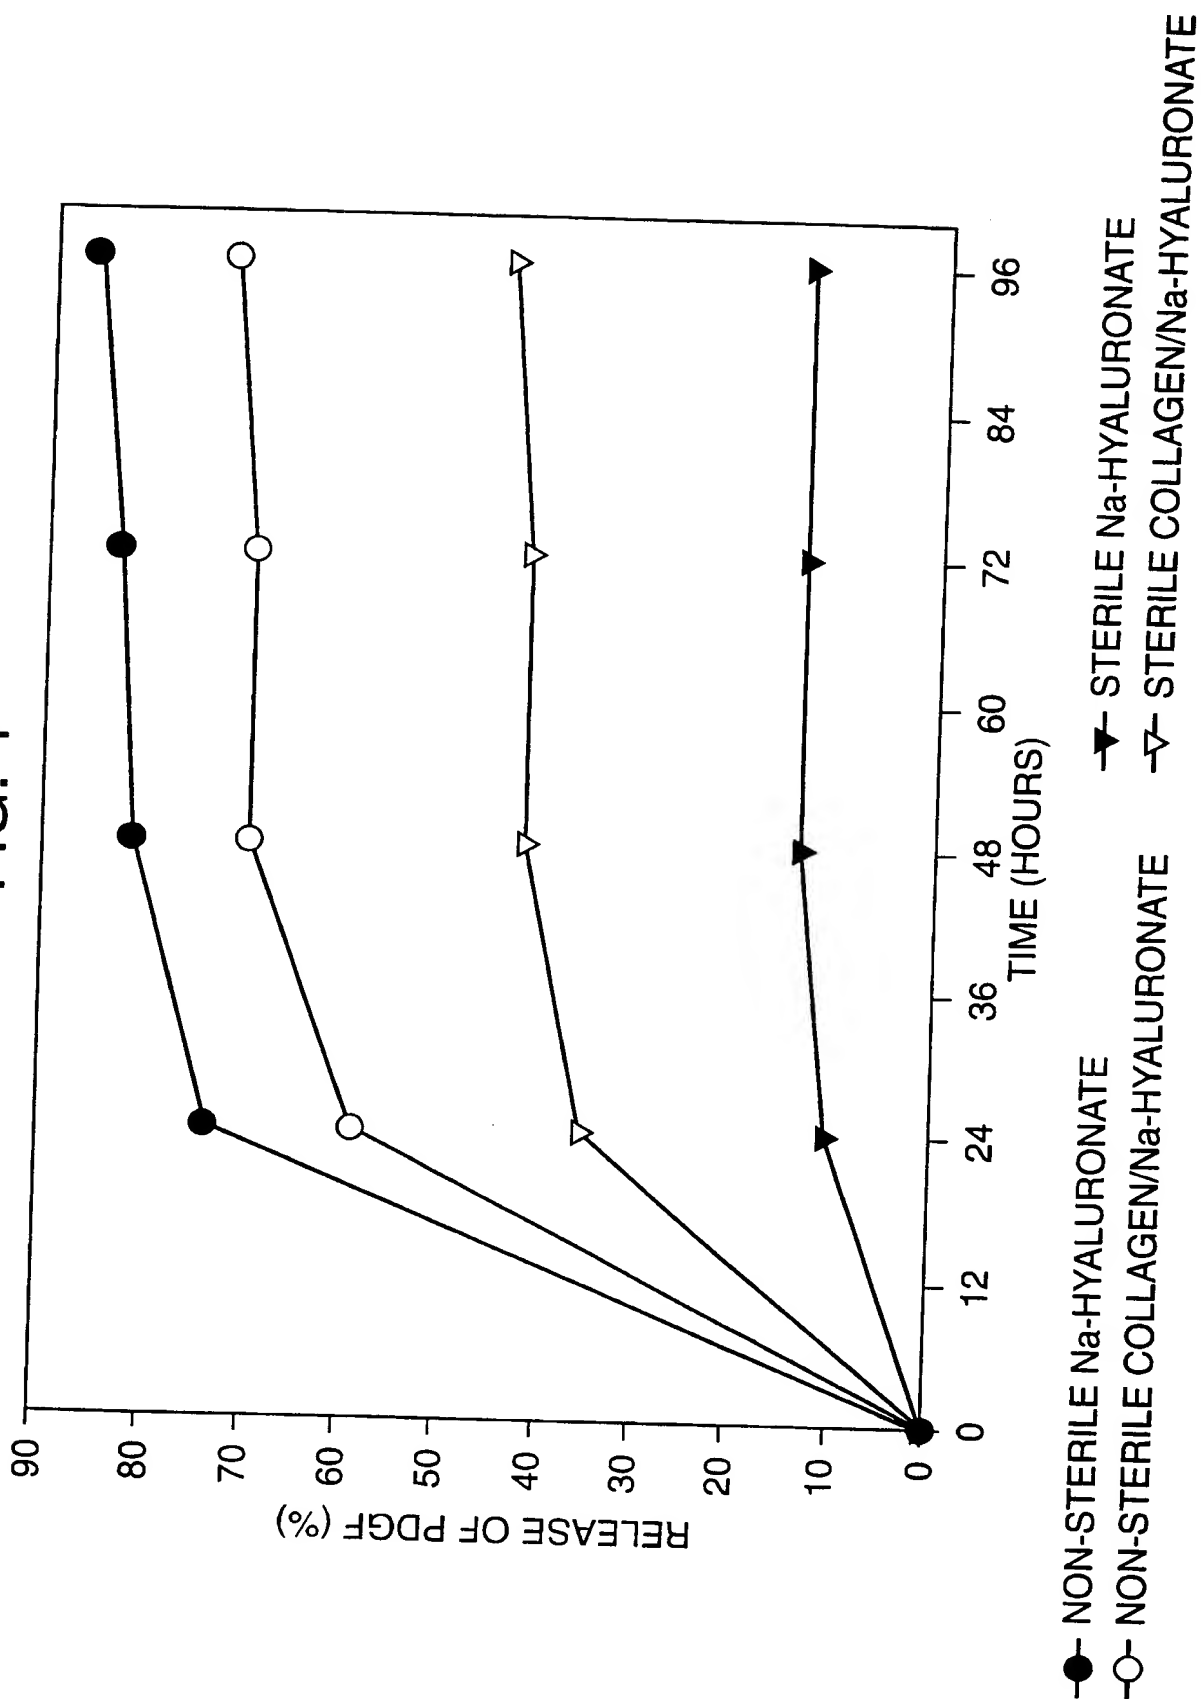


FIG. 5

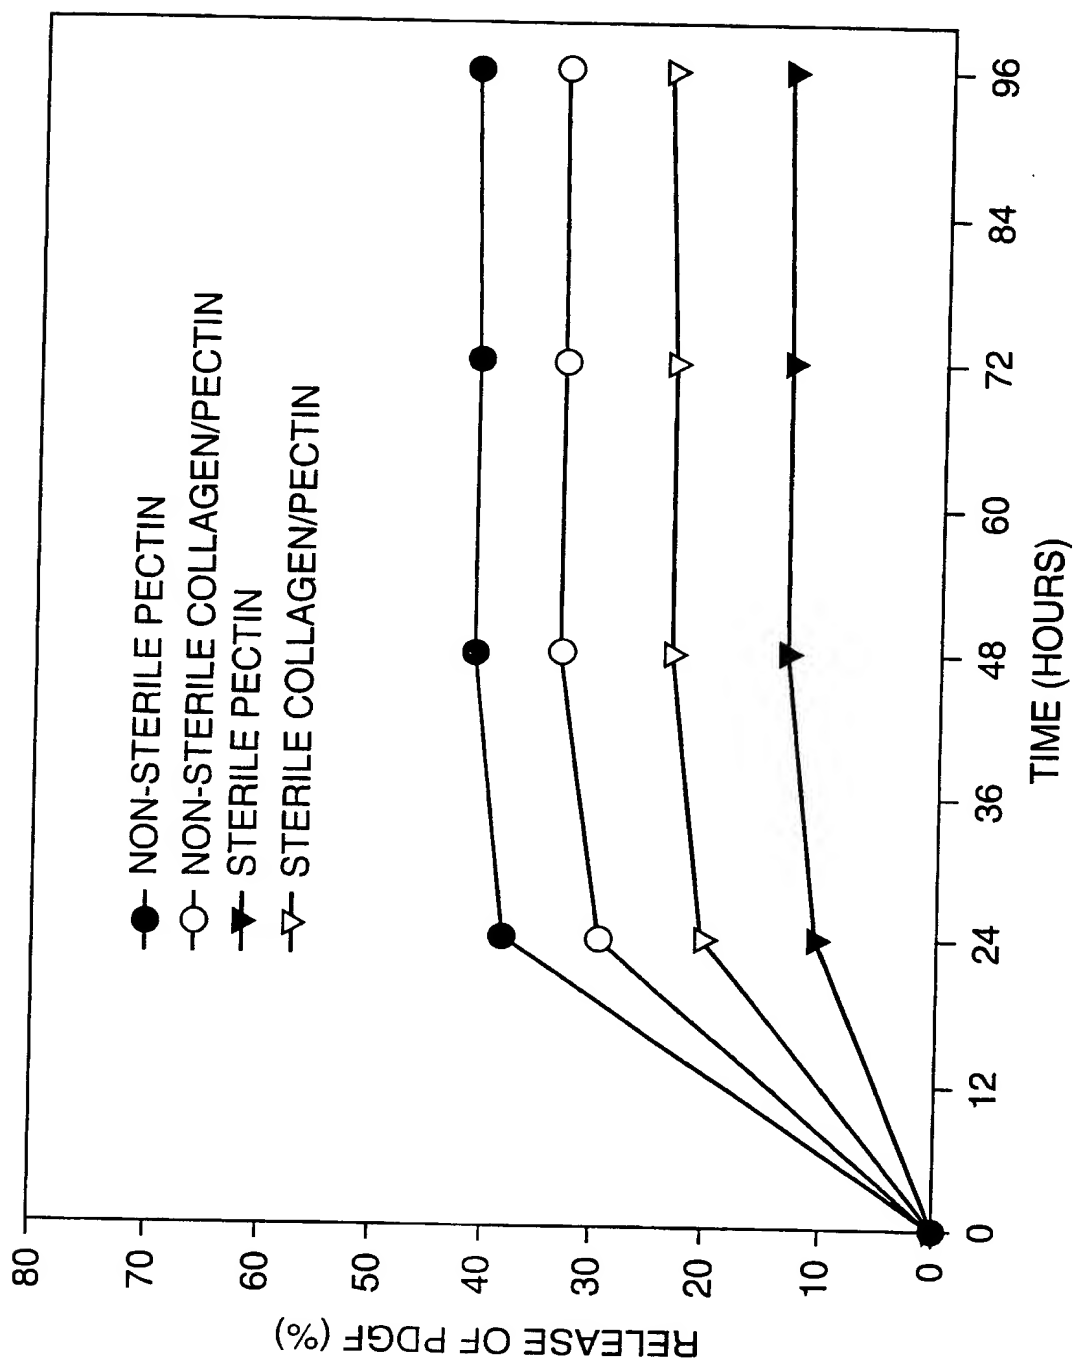

- NON-STERILE LOCUST BEAN GUM
- NON-STERILE COLLAGEN/LOCUST BEAN GUM
- ▼ STERILE LOCUST BEAN GUM
- ▽ STERILE COLLAGEN/LOCUST BEAN GUM

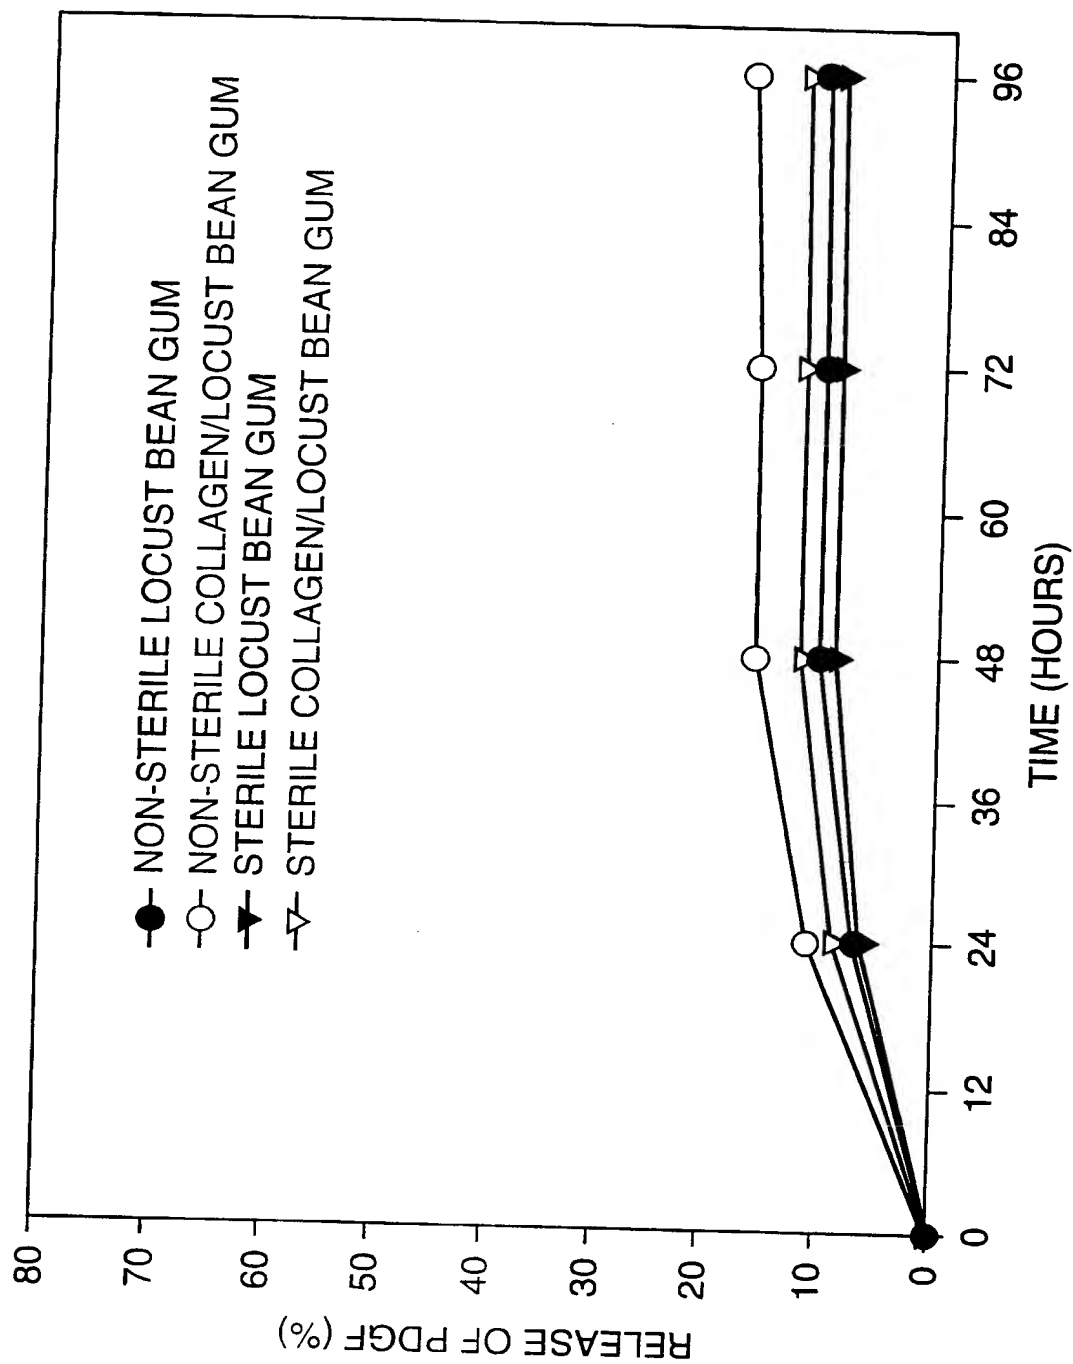


FIG. 7

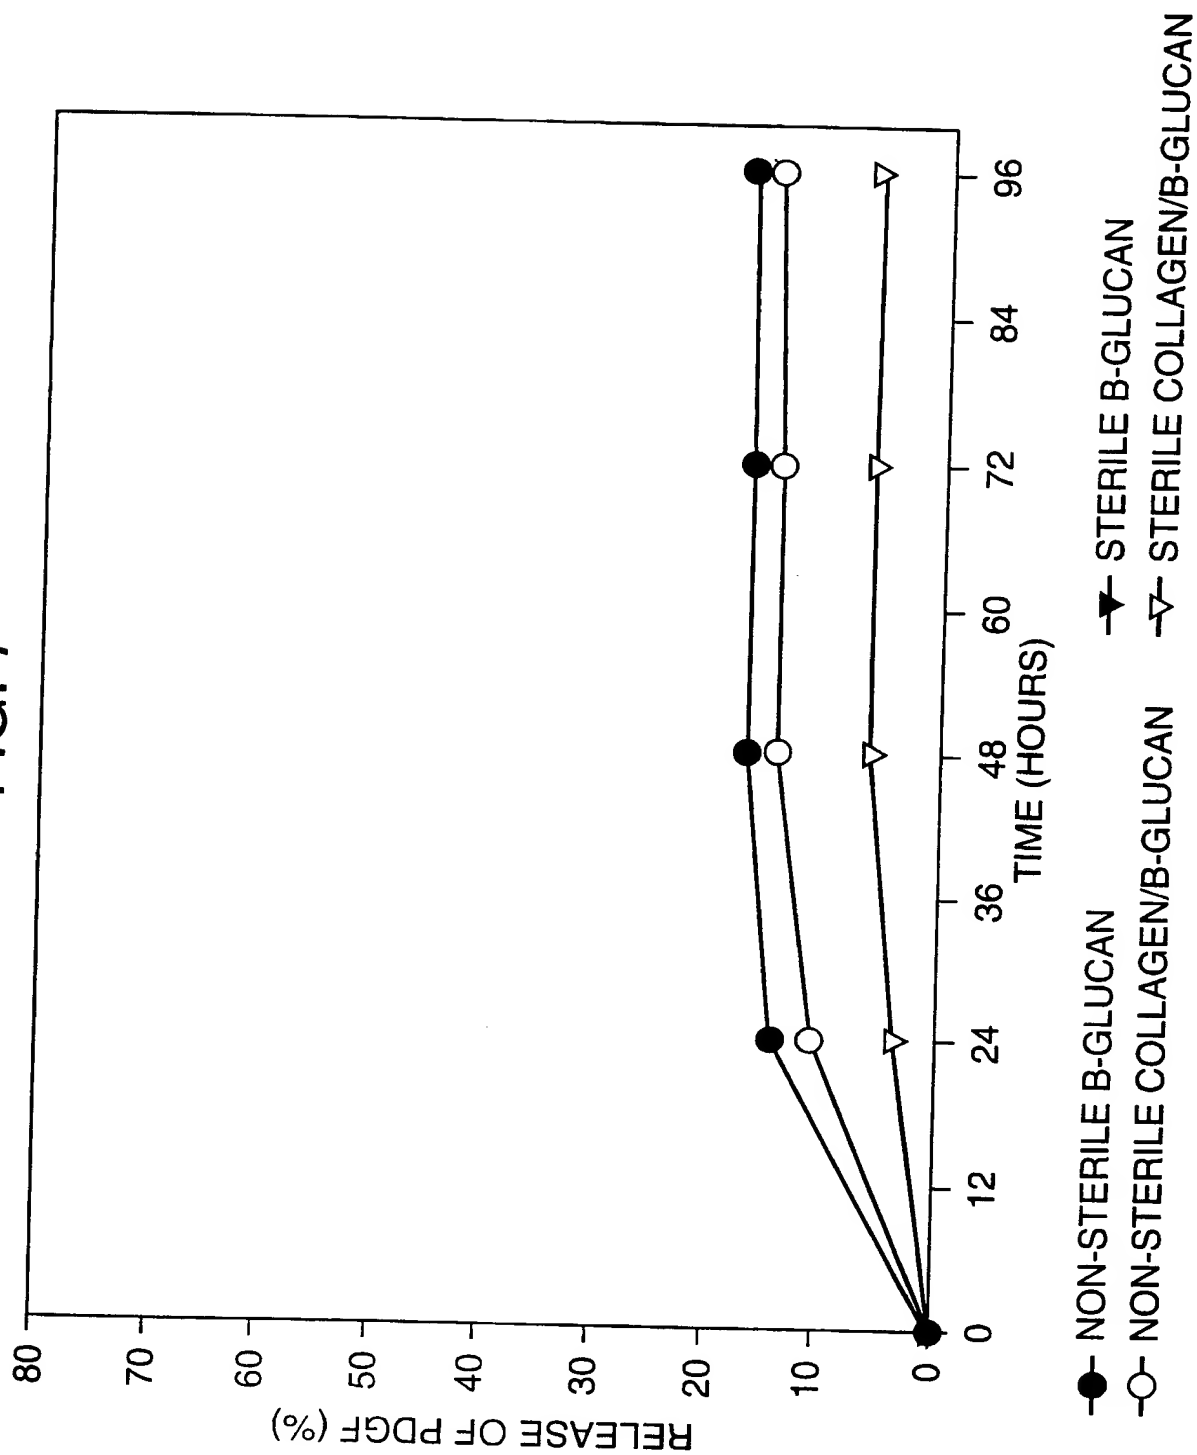


FIG. 8

